

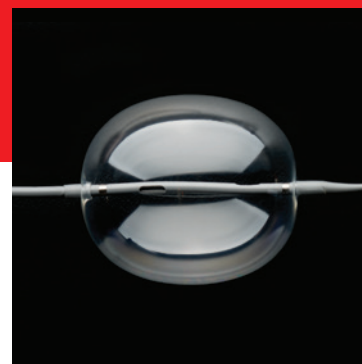


# THE NEXT GENERATION

in aortic accessories

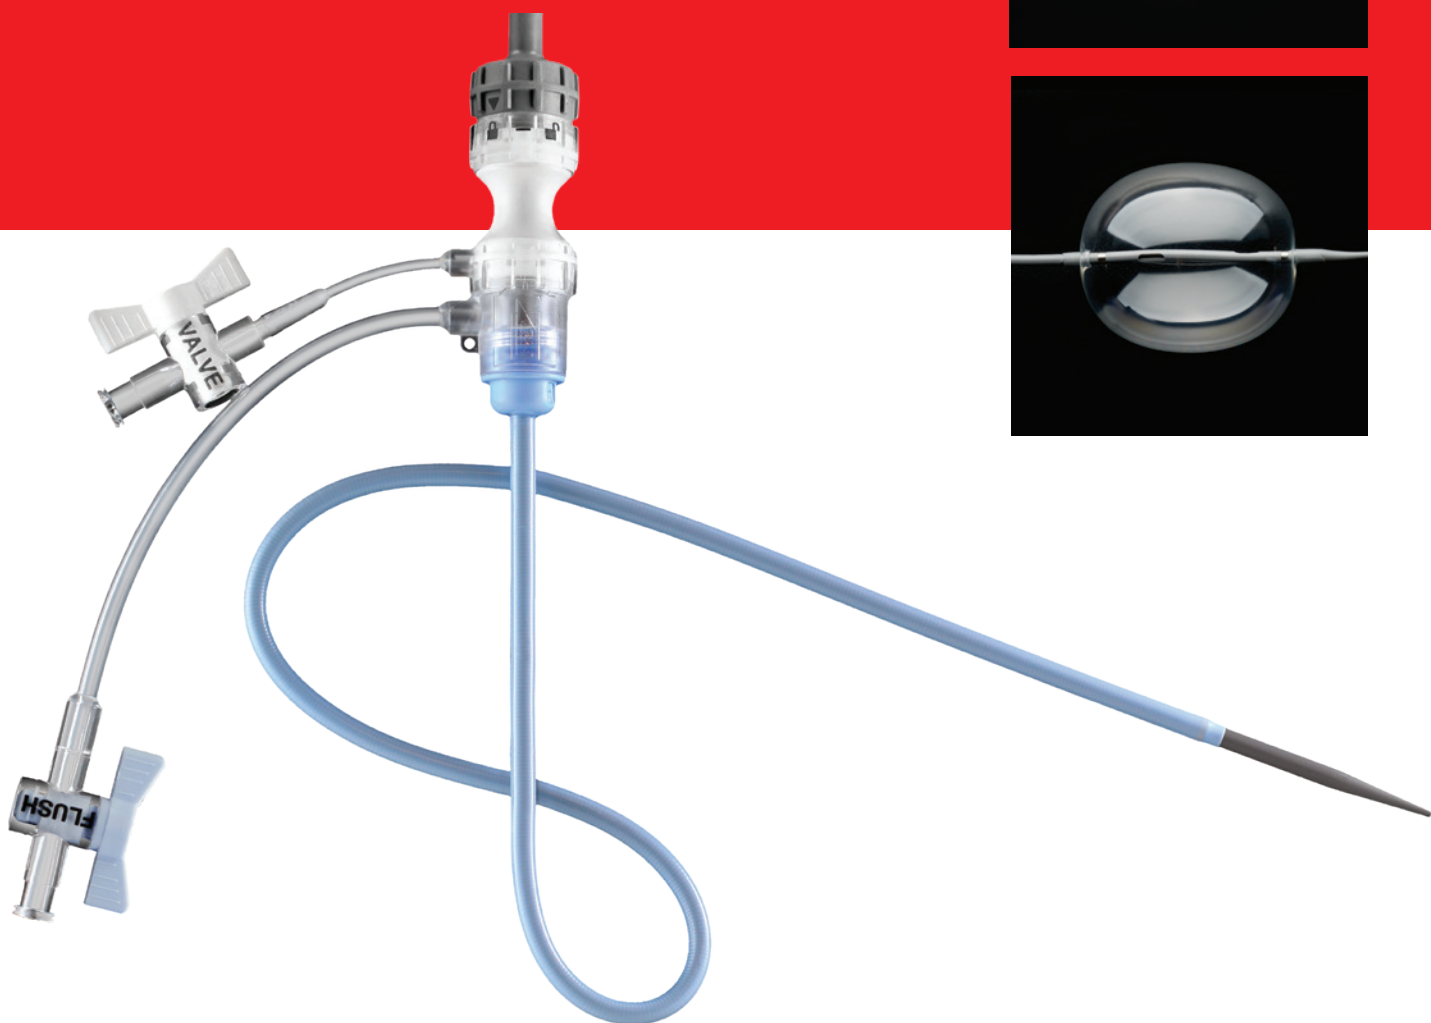

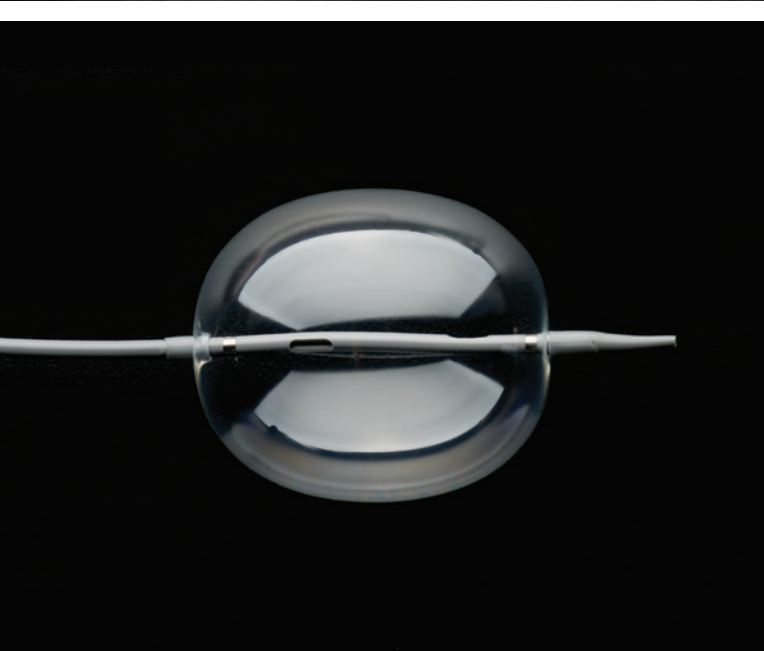

Each accessory plays a key role in supporting our best-in-class EVAR and TEVAR devices, promoting positive outcomes.

## GORE® DrySeal Flex Introducer Sheath

- **Deliver with ease:** Hydrophilic coating and enhanced flexibility provide exceptional access to challenging anatomies and branch vessels
- **Minimize blood loss:** Exclusive DrySeal valve enables introduction of multiple devices with proven hemostasis control
- **Care for more patients:** Optimized profile and configurations provide tailored delivery options for a broader range of patient anatomy
- **Complete confidence:** Engineered for use with our endovascular portfolio

## GORE® Molding & Occlusion Balloon Catheter

- **Optimize seal:** Proven radial expansion force across the range of EVAR device sizes (10–37 mm)
- **Minimize risk:** Engineered with the lowest profile to reduce access-related complications
- **Enhance control:** Designed for excellent pushability and trackability with uncompromised inflation / deflation time

## GORE® Tri-Lobe Balloon Catheter

- **Continuous blood flow:** Unique design allows flow around the lobes while inflated
- **Decreased hemodynamic pressure** on the inflated balloons with approximately 80% of flow for distal perfusion<sup>1</sup>
- **Minimizes potential for endoprosthesis movement** and blood pressure spikes post deployment due to significantly reduced hemodynamic pressures<sup>2</sup>
- **Rapid, uniform, and simultaneous** inflation and deflation

1. Bloss R, Krall B. *Balloon Testing on Pulse Duplicator*. Flagstaff, AZ: W. L. Gore & Associates, Inc.; 2009. [Technology notebook]. 1088.

2. Gendron M. *Simulated Use Testing of Aortic Balloon Catheter for Design Verification – Final Amendment*. Flagstaff, AZ: W. L. Gore & Associates, Inc; 2008. [Work plan]. MD39672.

## GORE® DrySeal Flex Introducer Sheath

Catalogue number	Sheath size (Fr)	Minimum sheath ID (mm)	Nominal sheath OD (mm)	Working length (cm)
DSF1233	12	4.0	4.7	33
DSF1245	12	4.0	4.7	45
DSF1433	14	4.7	5.3	33
DSF1533	15	5.0	5.6	33
DSF1633	16	5.3	6.1	33
DSF1833	18	6.0	6.7	33
DSF2033	20	6.7	7.5	33
DSF2065	20	6.7	7.5	65
DSF2233	22	7.3	8.2	33
DSF2265	22	7.3	8.2	65
DSF2433	24	8.0	8.8	33
DSF2465	24	8.0	8.8	65
DSF2633	26	8.7	9.5	33
DSF2665	26	8.7	9.5	65

## GORE® Tri-Lobe Balloon Catheter

Catalogue number	Inner vessel diameter (mm)
BCM1634	16–34
BCL2645	26–42

## GORE® Molding & Occlusion Balloon Catheter

Catalogue number	Size (Fr)	Balloon diameter (mm)	Catheter length (cm)
MOB37	10	10–37	90



### W. L. GORE & ASSOCIATES, INC.

Flagstaff, AZ 86004

+65.67332882 (Asia Pacific)

00800.6334.4673 (Europe)

800.437.8181 (United States)

928.779.2771 (United States)

[goremedical.com](http://goremedical.com)

Products listed may not be available in all markets.

GORE® and designs are trademarks of W. L. Gore & Associates.

© 2010, 2012, 2013, 2018, 2019 W. L. Gore & Associates, Inc. AR0279-EN3 JANUARY 2019